



Glover et al.
USSN:
Filed:

Mark Joy
Leydig, Voit & Mayer

Sheet 1 of 3
09/869,637
01/15/02
(312) 616-5600
Ref. # 218499

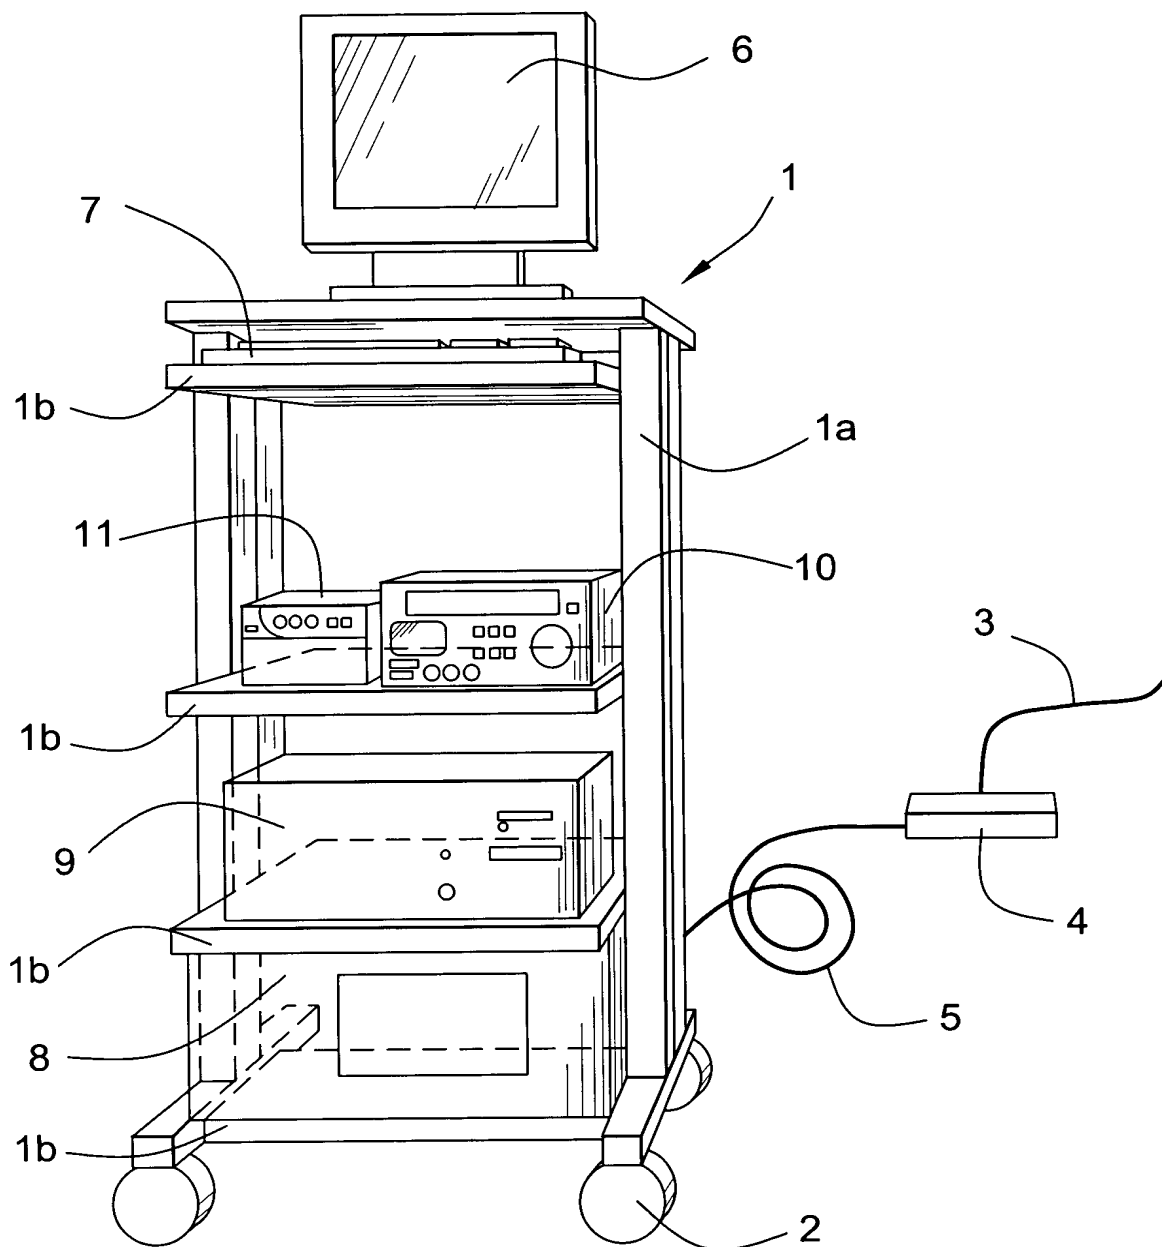


FIG. 1
(PRIOR ART)


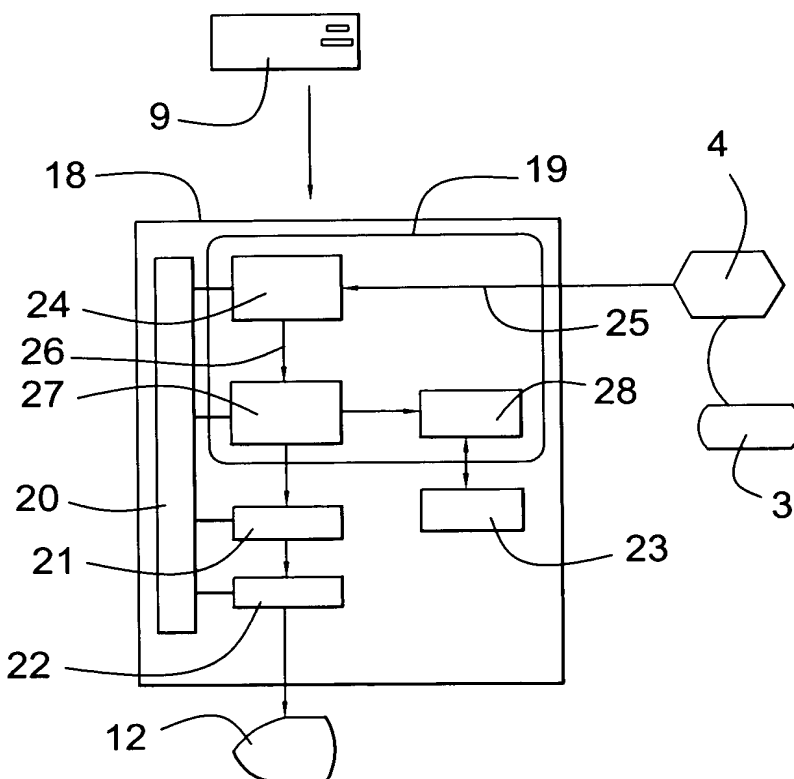


Figure 1 is a perspective view of a mobile device 10. The device includes a display 12 and a base 4. A cable 14 is connected to the base 4.

Diagram illustrating the setup of IVUS (Intravascular Ultrasound) components in an X-ray room. The diagram shows a patient table (4) with a catheter (12) inserted into a vessel. The catheter is connected to a control unit (13) and a monitor (14). The control unit is connected to a computer system (9) via a cable (15). The monitor displays the IVUS image (16) and is connected to the control unit via a cable (17). The diagram is labeled "KEY IVUS SPECIFIC COMPONENTS" and "X-RAY ROOM".

FIG. 4



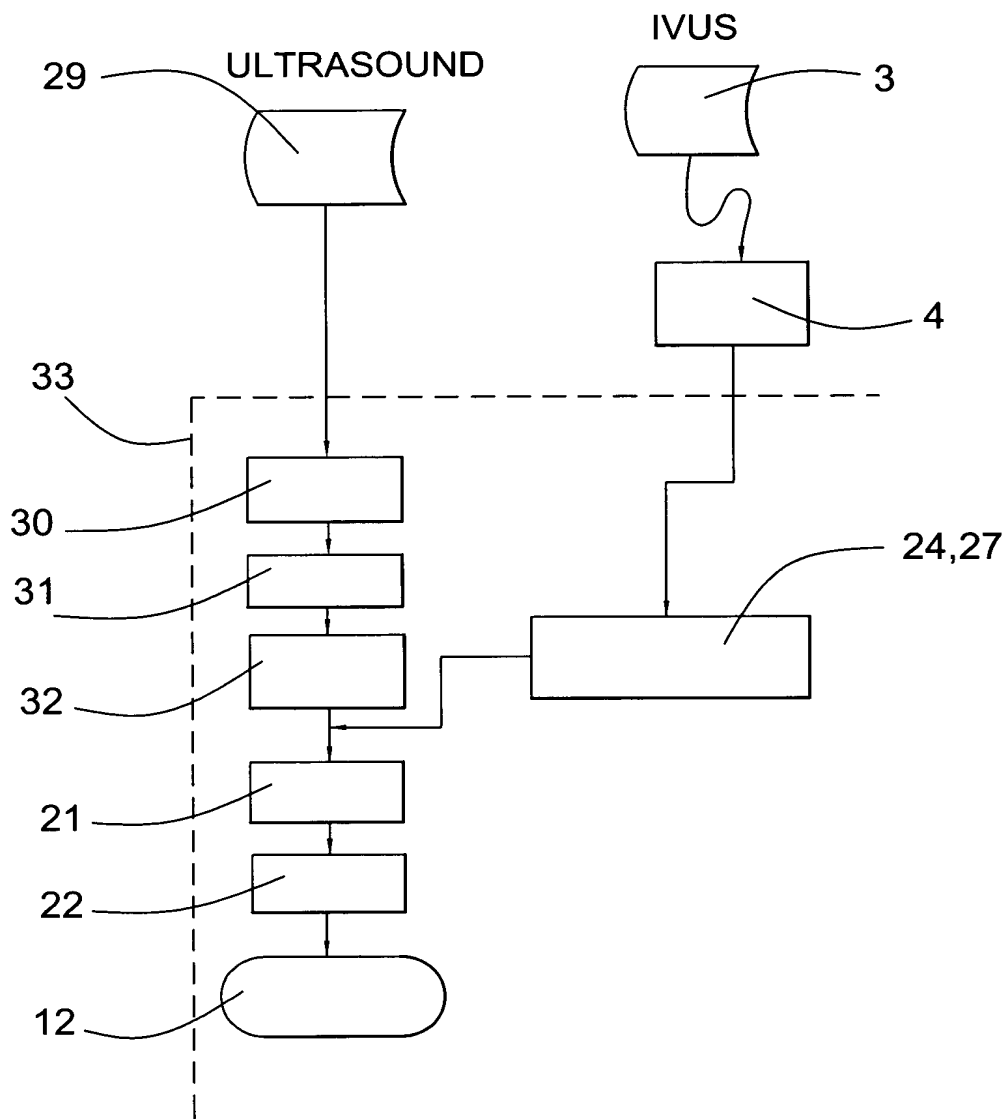


FIG. 5